

**Technical data****Analyser**

| | |
|-------------------------------|---|
| Housing: | steel sheet housing, 19" format, IP 40; 480 mm x 220 mm x 350 mm (w x h x d), weight approx. 28 kg |
| Measuring methods: | - bi-frequency measuring method (NO ₂ , SO ₂ , HF*, H ₂ O, CO ₂) - gas filter correlation (CO, NO, HCl, NH ₃ , N ₂ O, CH ₄) - zirconium dioxide cell (O ₂) |
| Number of meas. components: | max. 12 infrared components (dependent on application) and oxygen |
| Accuracy: | < 2% of the respective measuring range |
| Zero point correction: | automatical |
| Sensitivity correction: | with test gas, once in 6 months (sensitivity tests as standard with a concentration of 80% of the measuring range) |
| Cross-sensitivity correction: | additive, multiplicative |
| Air pressure correction: | yes |
| Standardisation: | dry, wet |
| Gas conveyance: | air-jet pump |
| Compressed-air connection: | 1...4 bar |
| Display/operating: | PC connection via USB (e.g. to the control panel in the analyser cabinet) |
| Interfaces: | 2 x RS232, USB |
| Power supply: | 110 V bis 230 V, 50/60 Hz, 300 W |
| Photometer: | - spectral range: 1...16 µm - gas path: continuously heated, standard 185 °C (higher temperatures on request) - path length of measuring cell: adjustable 2...10 m - dead volume of measuring cell: < 1 l - particle filter: 2 µm |

Analyser cabinet

| | |
|--------------------|---|
| Dimensions: | steel sheet cabinet, 800 mm x 2100 mm x 600 mm (w x h x d) |
| Weight: | approx. 200...300 kg (depending on fitments) |
| Display/operating: | integrated 15" control panel with touch surface, 1024 x 768 Pixel |

System

| | |
|-----------------------------|--|
| Ambient temperature: | 5...40 °C |
| Relative humidity: | max. 90% (non-condensing) |
| Compressed-air connection: | 4...6 bar (dependent on application) |
| Compressed-air consumption: | approx. 1 m ³ /h (dependent on application) |
| Calibration: | - zero point: automatical with instrument air - span point: with test gas, optionally automatical |
| Interfaces: | analogue outputs, Modbus, Profibus, further on request |
| Inputs: | for analogue and digital signals |
| Digital outputs: | failure, maintenance, maintenance requirement, measuring range switch-over, other |
| Analogue output: | 4 ... 20 mA |
| Remote control: | Ethernet, analogue modem |
| Power consumption: | 350 W |
| Power supply: | 230 V or 400 V / 50 Hz, 4000 W (analyser cabinet, air conditioner, probe) + 100 W/m measuring gas pipe |
| Suitability test: | DIN EN 15267, QAL1, Cert.-No.: 1729865-ts; DIN EN 15267-3; certification: MCERTS, Cert.-No.: Sira MC140256/01; DIN EN 15267-3, TA Luft, 17 th , 27 th BImSchV (as system part) |

Special models are possible on request.

* MCERTS certified according to DIN EN 15267-3

**MCA 10 HWIR****Product Information**

The multi component analyser MCA 10 HWIR serves the continuous emission measurement of pollutants in flue gas (e.g. CO, NO, N₂O, NO₂, NH₃, CH₄, HCl, SO₂, HF*; as system additionally TOC) and the measurement of CO₂, H₂O and O₂ as well as the continuous process control.

The device is suitability tested according to DIN EN 15267-3 and certified in compliance with QAL1 as well as MCERTS Performance Standards. As a part of the analyser system MCA 10 HWIR it is suitability tested and certified for systems after "TA Luft", 17th and 27th BImSchV according to DIN EN 15267-3.

Application

The MCA 10 HWIR is applicable all-purpose for measurement of emissions, raw gases or processes. As system in regulatory and operational emission measurement systems, amongst others, it serves the exhaust concentration control in combustion plants with different types of fuel, the thermal waste treatment, the combustion optimisation and the process management control.

Application examples:

- Power plants
- Waste incineration plants
- Refineries
- Cement industry
- Industrial exhaust air
- Paper mills
- Glass industry
- Chemical industry

**Function**

By the functional principle of the multi component analyser MCA 10 HWIR up to twelve infrared gas components can be detected simultaneously. As measuring methods bi-frequency measuring method and gas filter correlation are applied. Optionally, an oxygen measurement via zirconium dioxide cell is possible.

The analyser evaluates internally all specification-depending required concentrations with all necessary compensations and standardisations. By a connected PC the visualisation and operating with device-own user software is executed. The operating surface is designed for one-click operating via touch function.



Optionally, the additional connections at the device can be used for connection of external devices (e.g. for measurement of total organic carbon or mercury).

Measuring ranges



| Component | Certification range | Measuring range 2 | Measuring range 3 |
|------------------|---------------------------|----------------------------|----------------------------|
| CO | 0...75 mg/m ³ | 0...300 mg/m ³ | 0...5000 mg/m ³ |
| CO ₂ | 0...25 vol. % | 0...50 vol. % | - |
| NO | 0...200 mg/m ³ | 0...400 mg/m ³ | 0...3000 mg/m ³ |
| NO ₂ | 0...50 mg/m ³ | 0...500 mg/m ³ | - |
| N ₂ O | 0...50 mg/m ³ | 0...3000 mg/m ³ | - |
| NH ₃ | 0...10 mg/m ³ | 0...50 mg/m ³ | 0...500 mg/m ³ |
| SO ₂ | 0...75 mg/m ³ | 0...300 mg/m ³ | 0...2500 mg/m ³ |
| HCl | 0...15 mg/m ³ | 0...90 mg/m ³ | 0...5000 mg/m ³ |
| HF* | - | 0...20 mg/m ³ | - |
| H ₂ O | 0...40 vol. % | - | - |
| CH ₄ | 0...50 mg/m ³ | 0...500 mg/m ³ | - |
| TOC | 0...15 mg/m ³ | 0...30 mg/m ³ | - |
| O ₂ | 0...25 vol. % | - | - |

Measuring methods


Bi-frequency measuring method

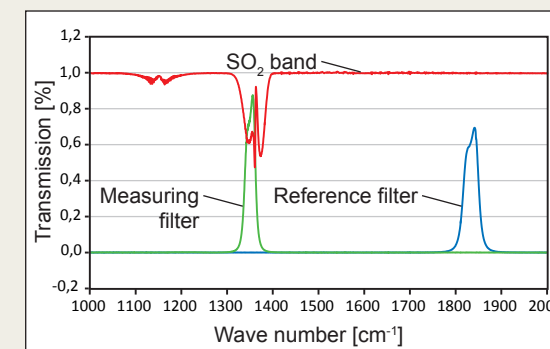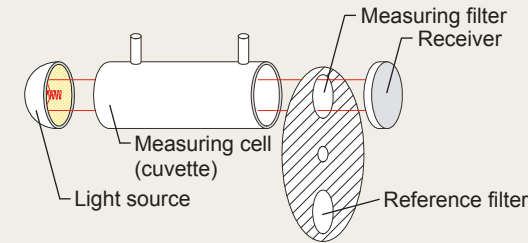

Gas filter correlation

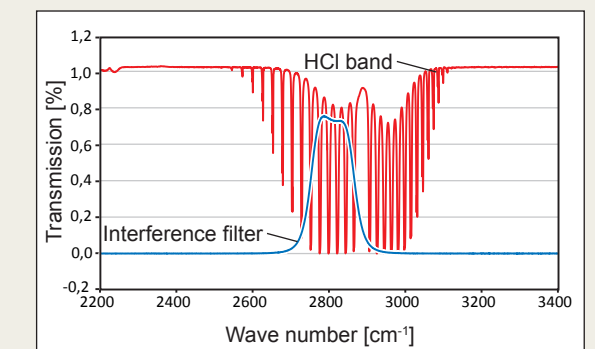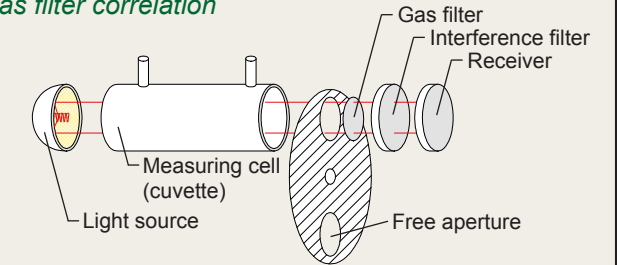


Design of CPU components

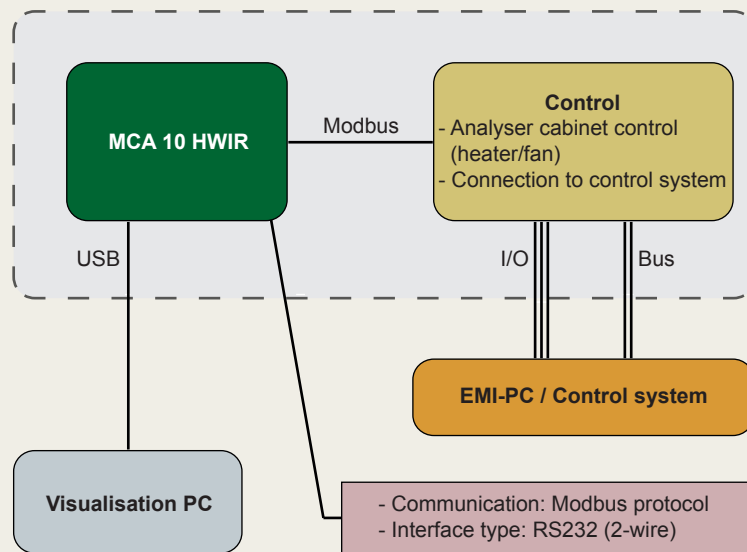

The system design consists basically of three logic units:

- Multi component analyser MCA 10 HWIR
- Visualisation PC with user software
- PLC control for analyser cabinet

System design

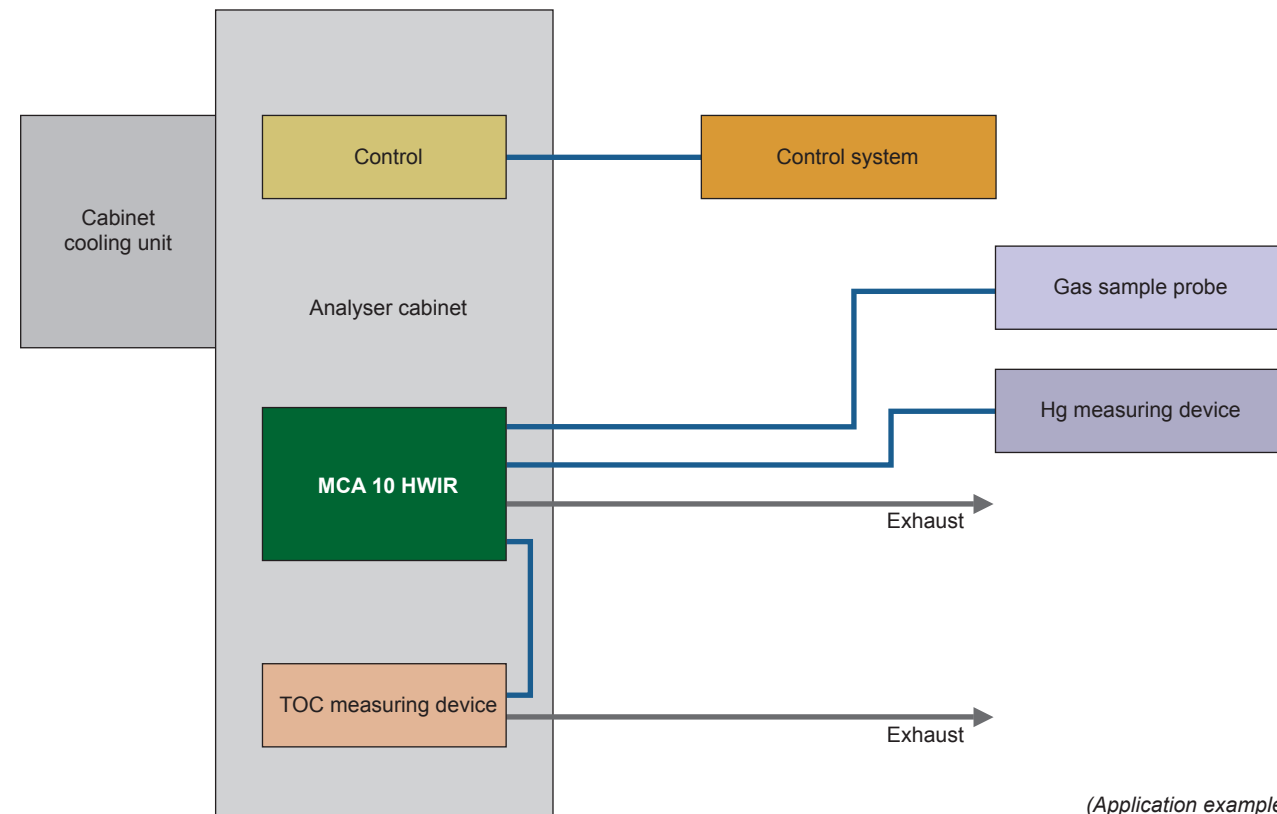

(Application example)

Highlights of the device

- modularly structured hot gas analyser system (without gas cooler)
- continuous, extractive measurement of up to twelve infrared components
- field-proven components, modern photometer technology
- long operation times, high reliability
- compact 19" insertion of the analyser → easy mounting
- easy system design
- pre-calibrated → immediately deployable
- integrated control
- integrated zero gas provision
- self control (additional control of inlet temperature)
- zero point drift control
- remote diagnosis and system setting via Ethernet
- first-class price-performance ratio